Fluorescence Intensity NORMAL MUCOSAL TISSUE with 370 nm excitation ADENOMA 0 L 400

Figure 1

550

Wavelength (nm)

600


650

700

450


500

Applicant(s): Stephen F. Fulghum, Jr.
itte: AUTOFLUORESCENCE IMAGING
SYSTEM FOR ENDOSCOPY
Docket No.: 301489.1003-113

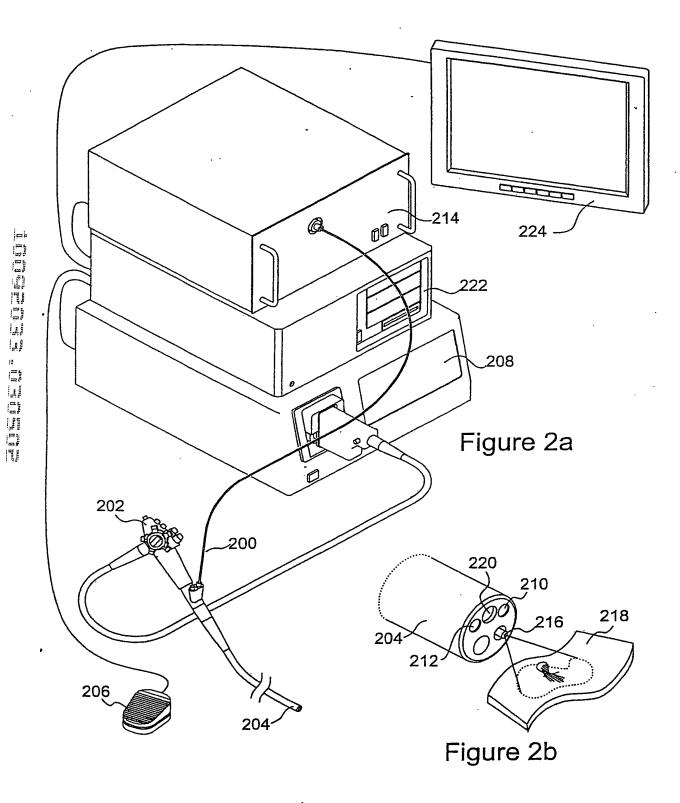


Applicant(s): Stephen F. Fulghum, Jr. litle: AUTOFLUORESCENCE IMAGING SYSTEM FOR ENDOSCOPY

Docket No.: 301489.1003-113

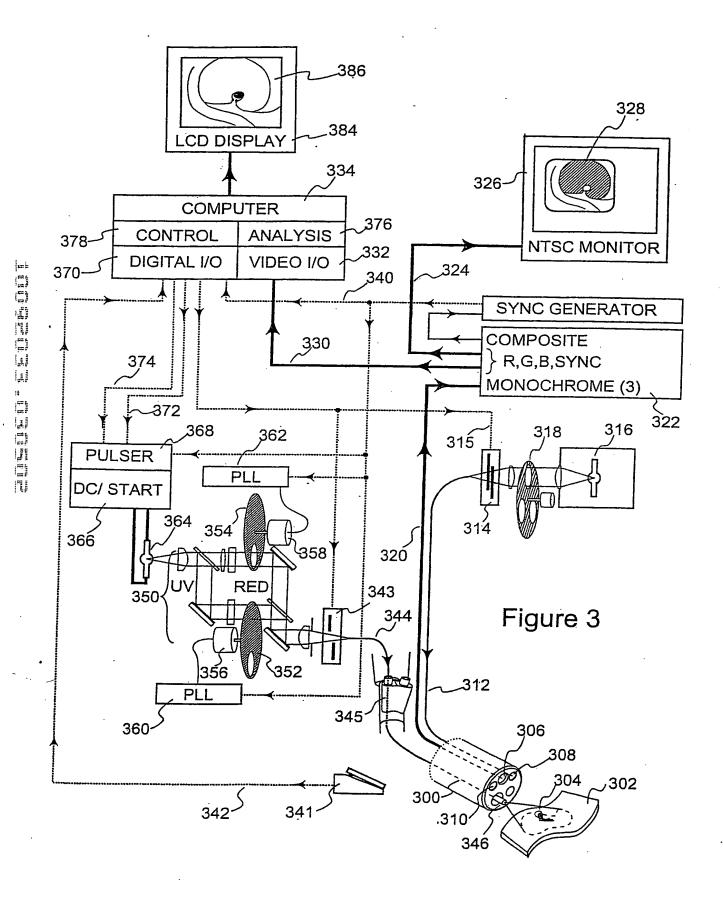

Applicant(s): Stephen F. Fulghum, Jr. itle: AUTOFLUORESCENCE IMAGING

SYSTEM FOR ENDOSCOPY Docket No.: 301489.1003-113

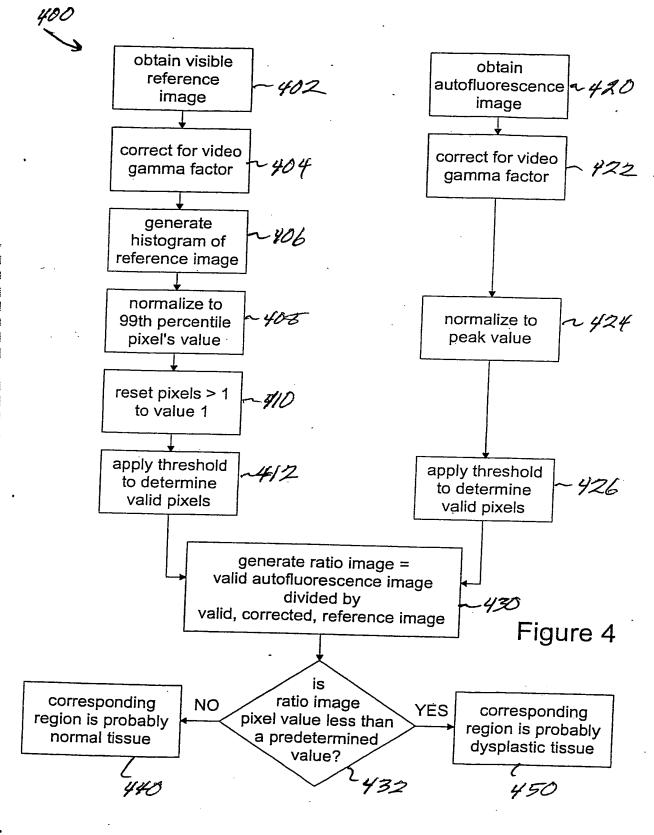


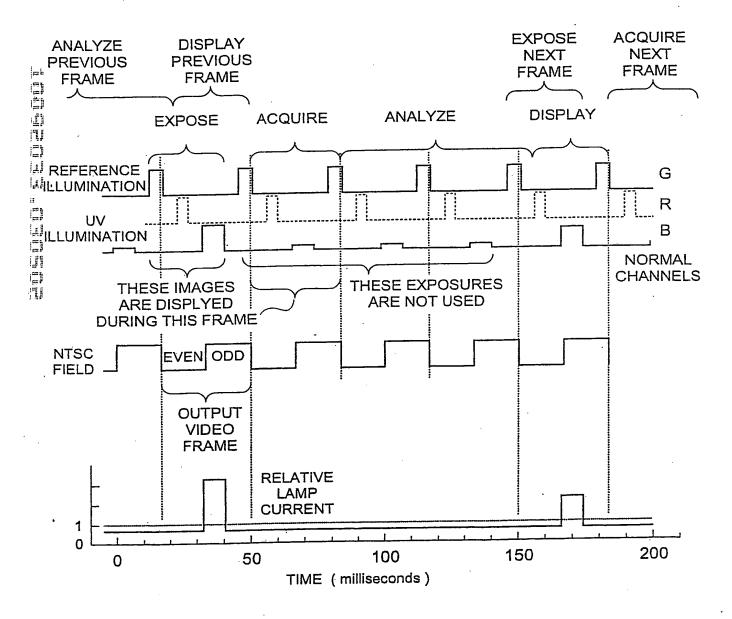


Figure 5


plicant(s): Stephen F. Fulghum, Jr. le: AUTOFLUORESCENCE IMAGING

SYSTEM FOR ENDOSCOPY Docket No.: 301489.1003-113

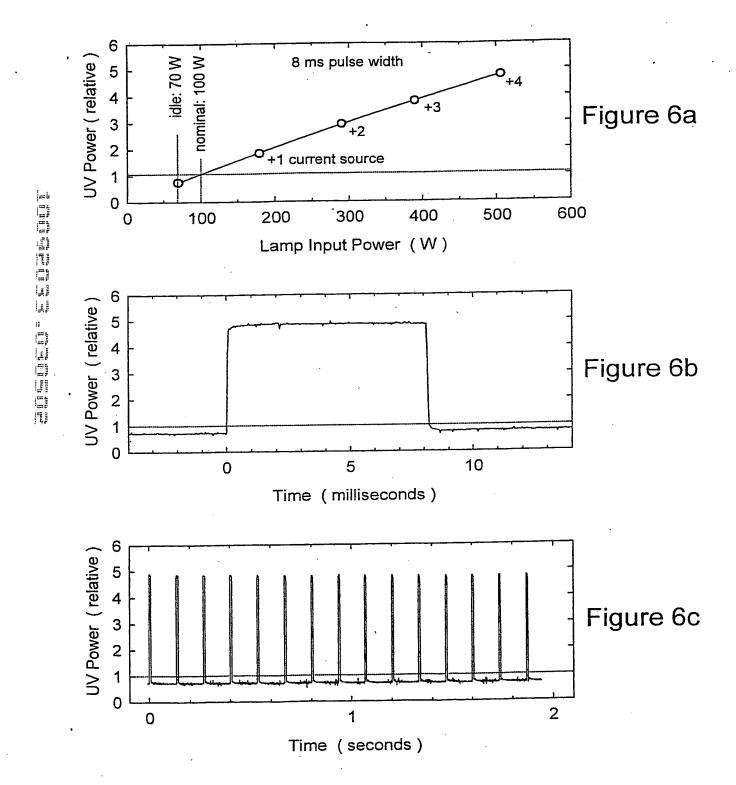


Applicant(s): Stephen F. Eulghum, Jr.
Title: AUTOFLUORESCENCE IMAGING

SYSTEM FOR ENDOSCOPY Docket No.: 301489.1003-113

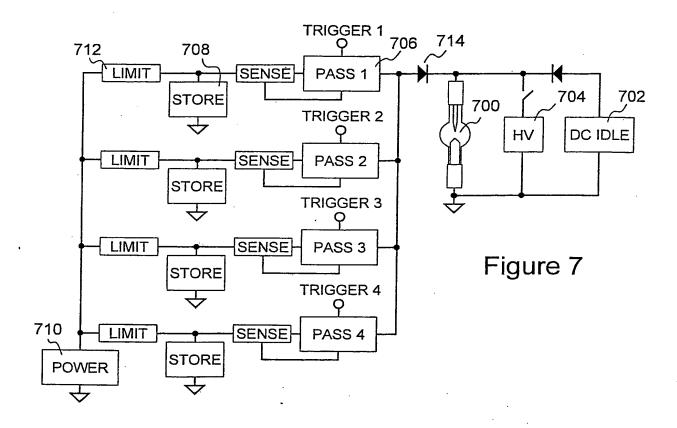

olicant(s): Stephen F-Fulghum, Jr. le: AUTOFLUORESCENCE IMAGING

SYSTEM FOR ENDOSCOPY Docket No.: 301489.1003-113

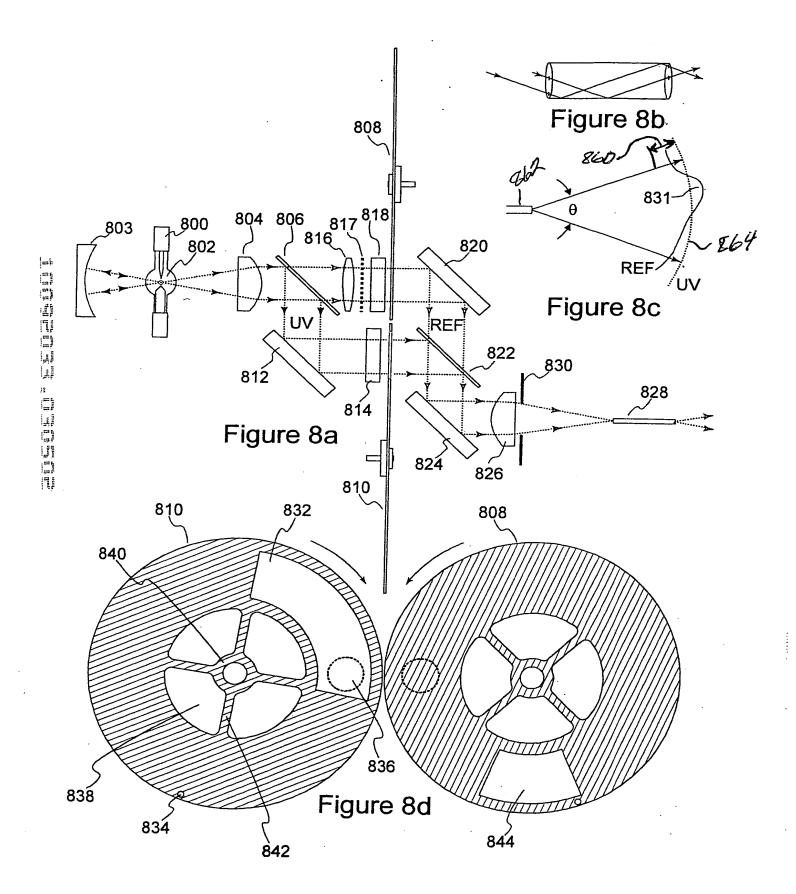

Applicant(s): Stephen F. Fulghum, Jr.
Title: AUTOFLUORESCENCE IMAGING
SYSTEM FOR ENDOSCOPY
Docket No.: 301489.1003-113



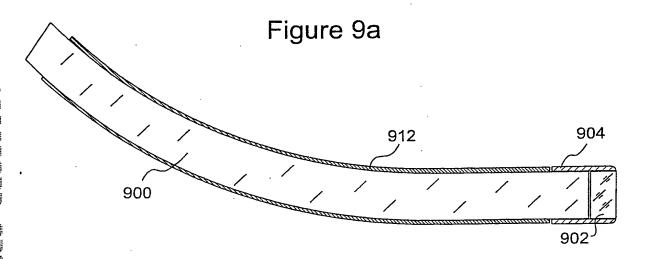


Figure 9b 




pplicant(s): Stephen F. Fulghum, Jr. tle: AUTOFLUORESCENCE IMAGING

SYSTEM FOR ENDOSCOPY Docket No.: 301489.1003-113

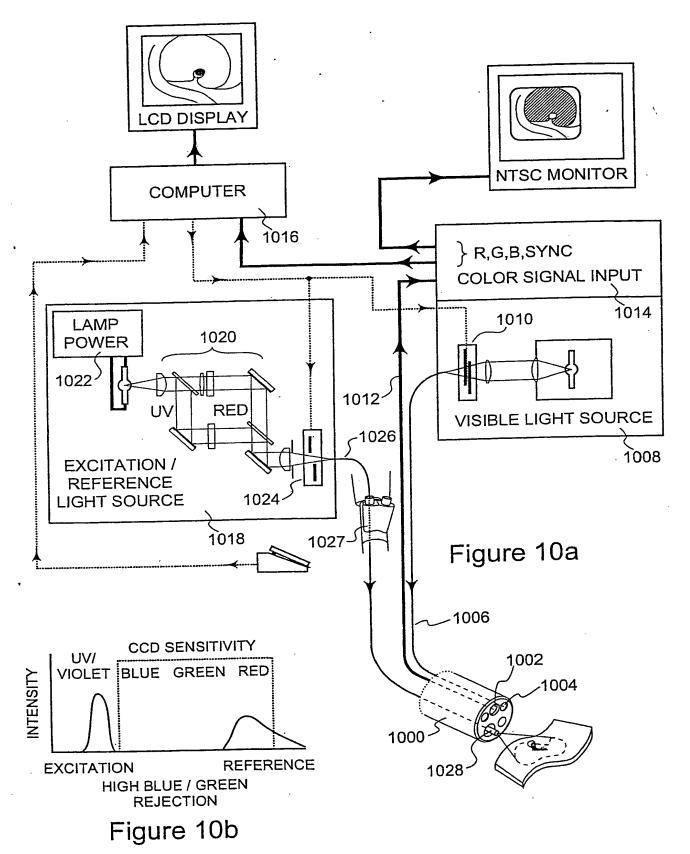

Docket No.: 301489.1003-113

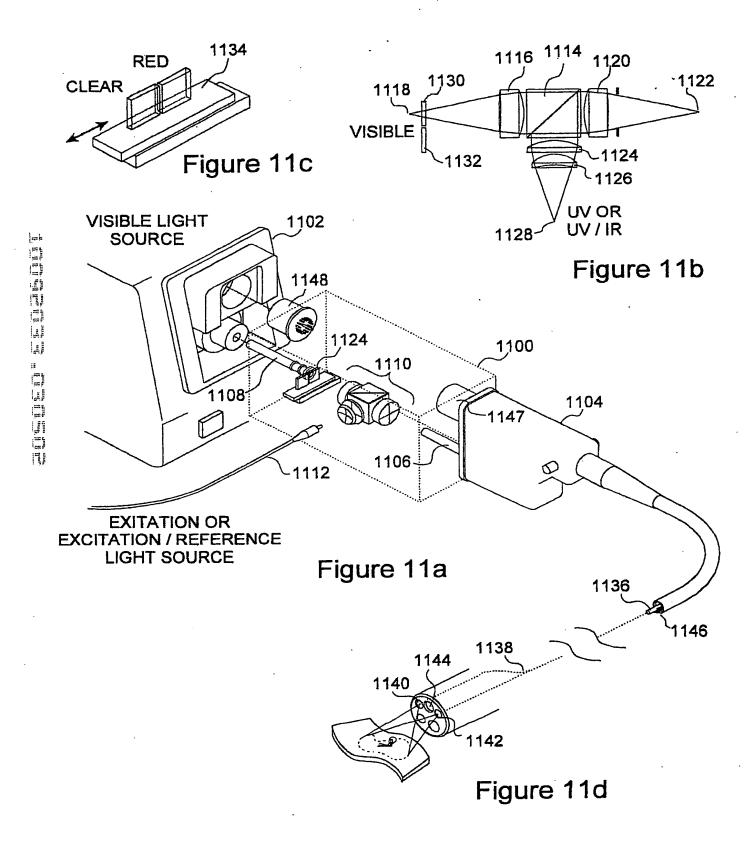

cant(s): Stephen F. Fulghum, Jr. AUTOFLUORESCENCE IMAGING

SYSTEM FOR ENDOSCOPY Docket No.: 301489.1003-113

